

FIG. 1

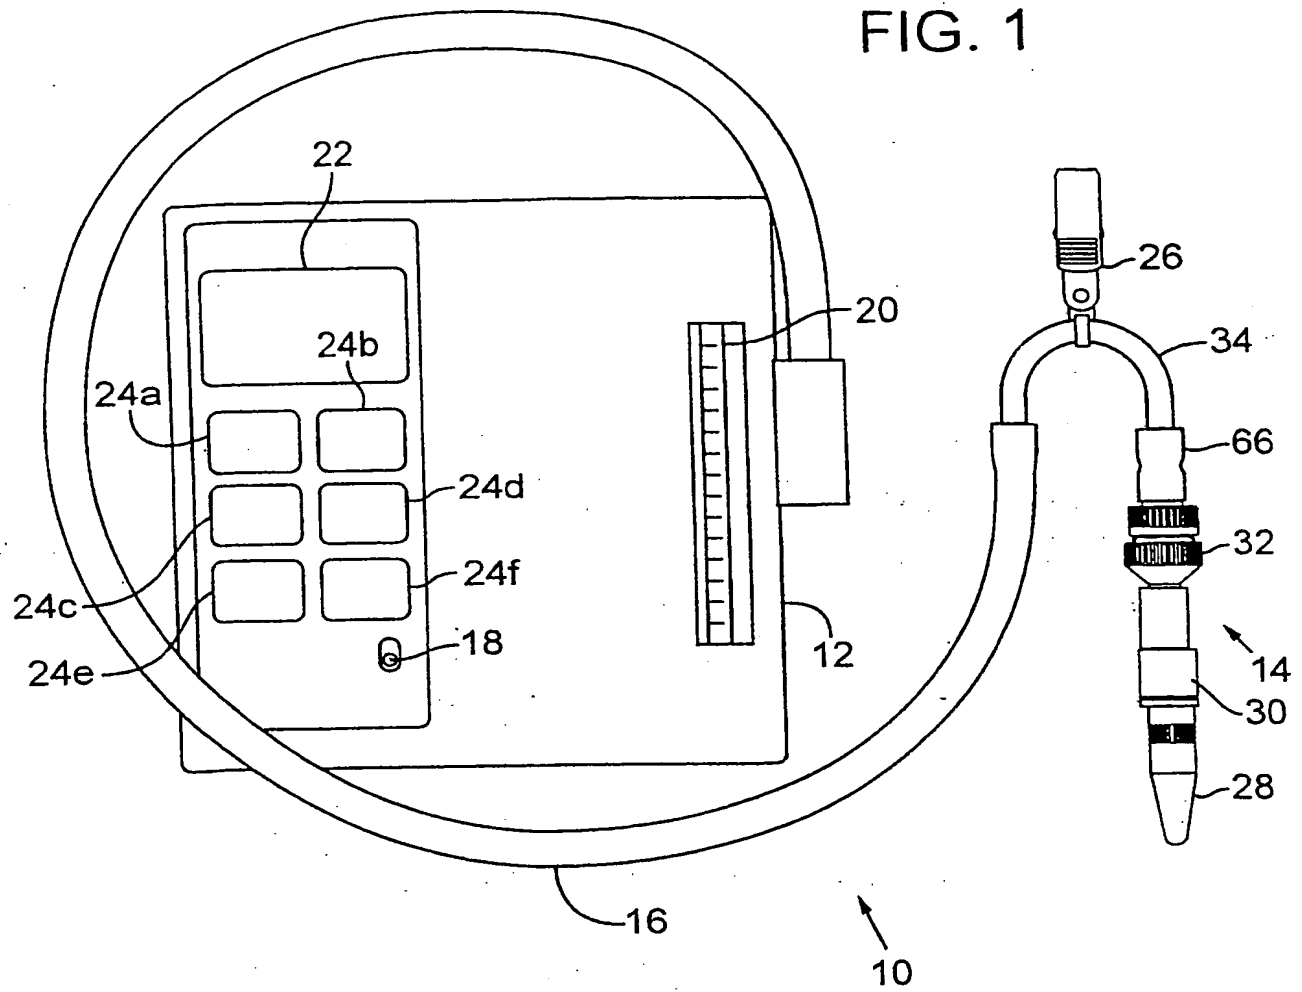


FIG. 2

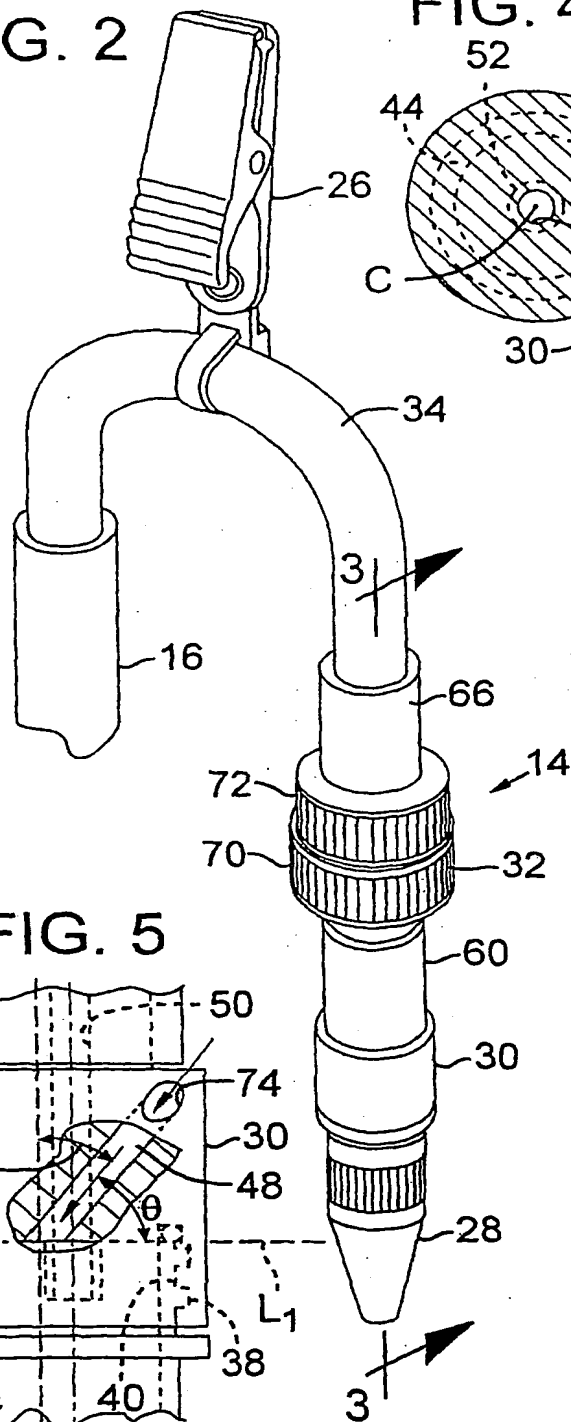


FIG. 4

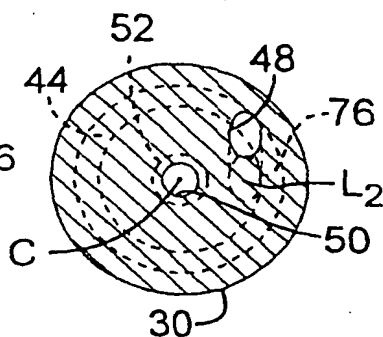


FIG. 3

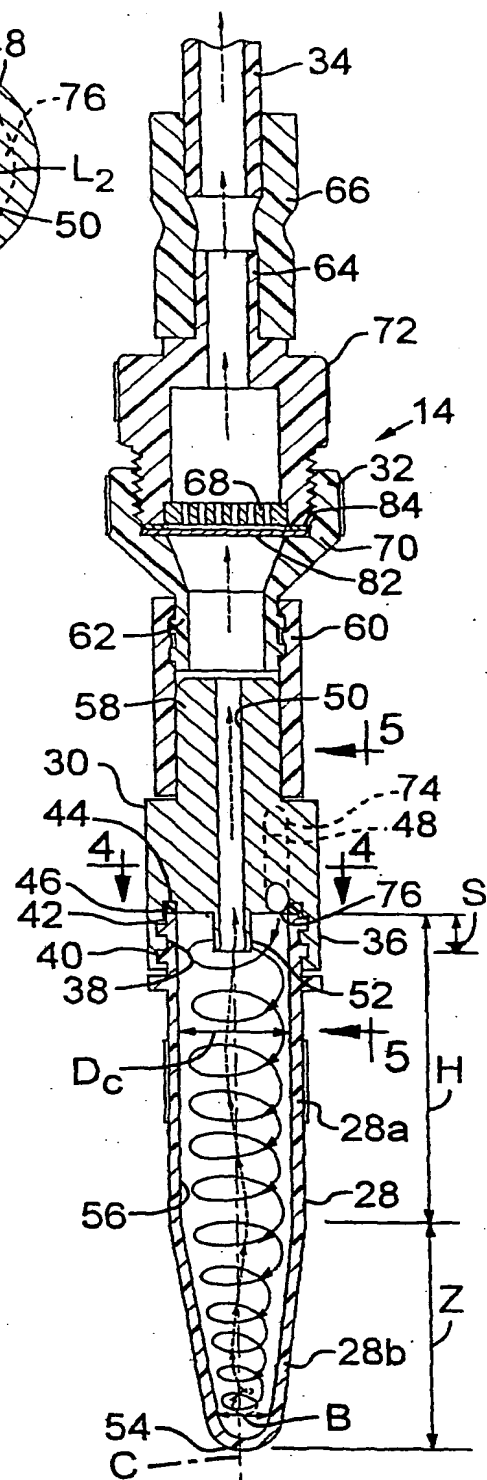


FIG. 5

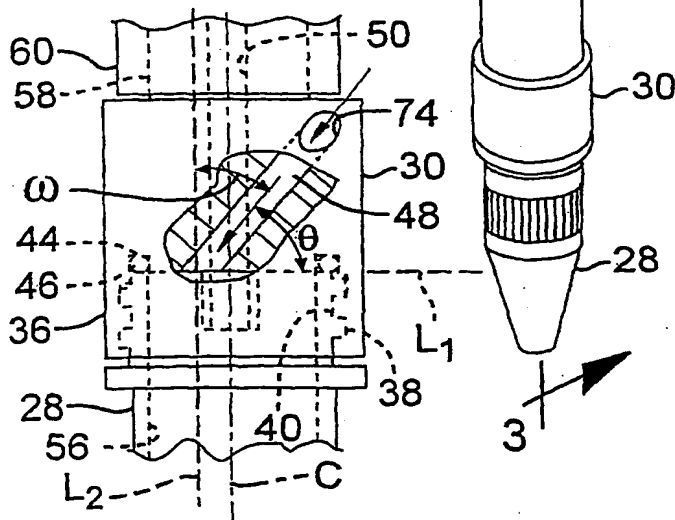


FIG. 6

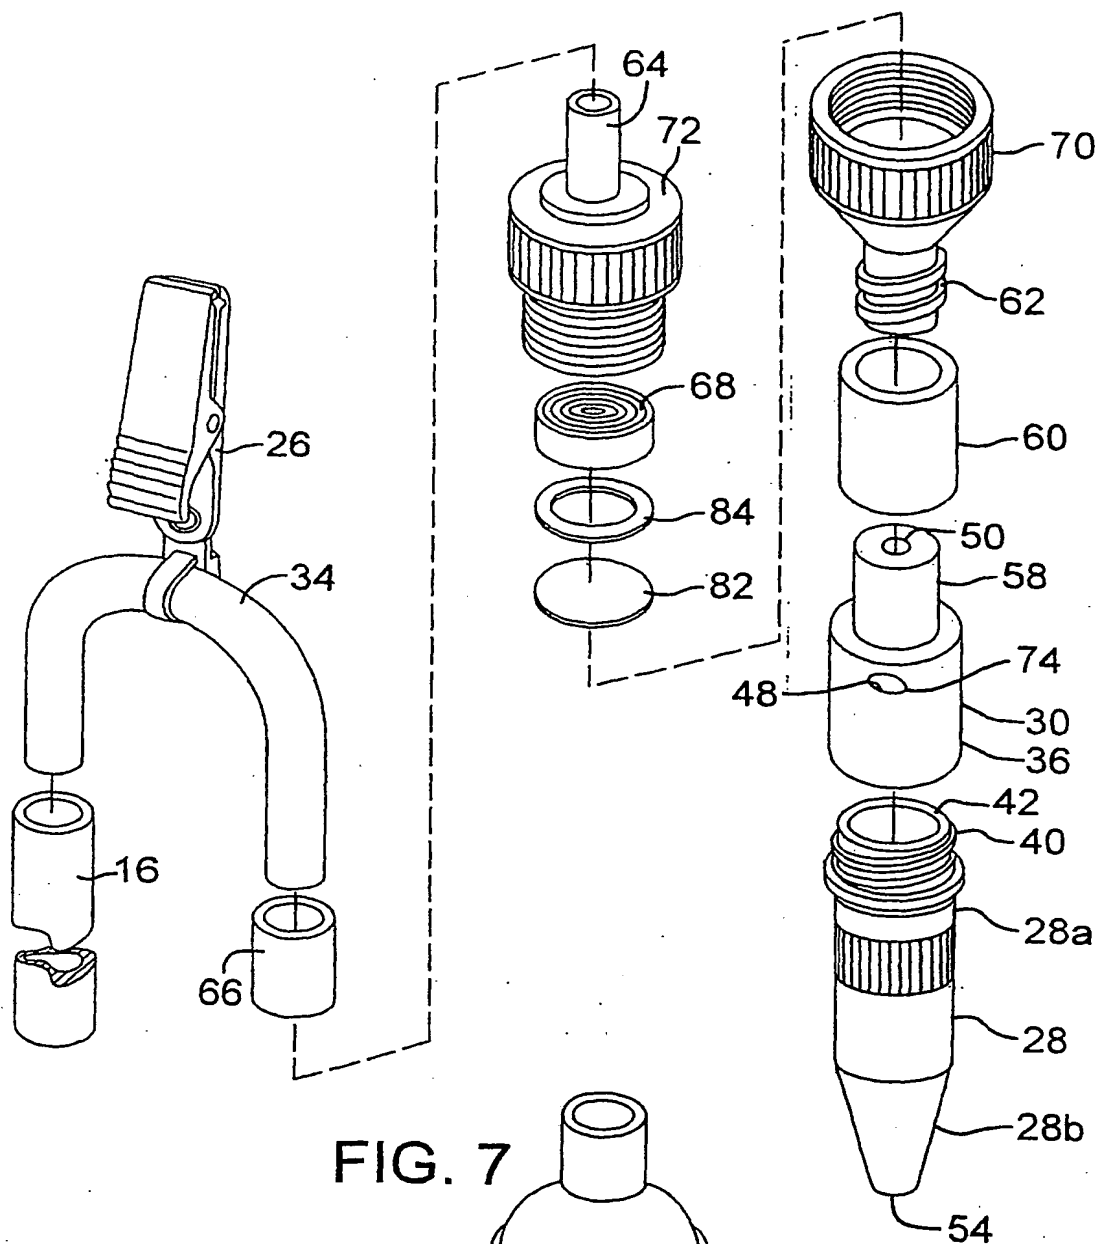


FIG. 7

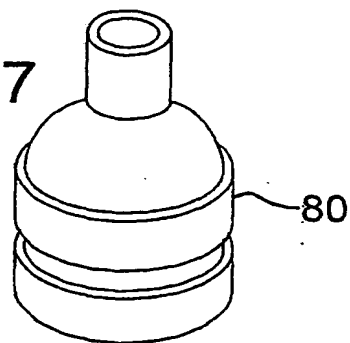


FIG. 8

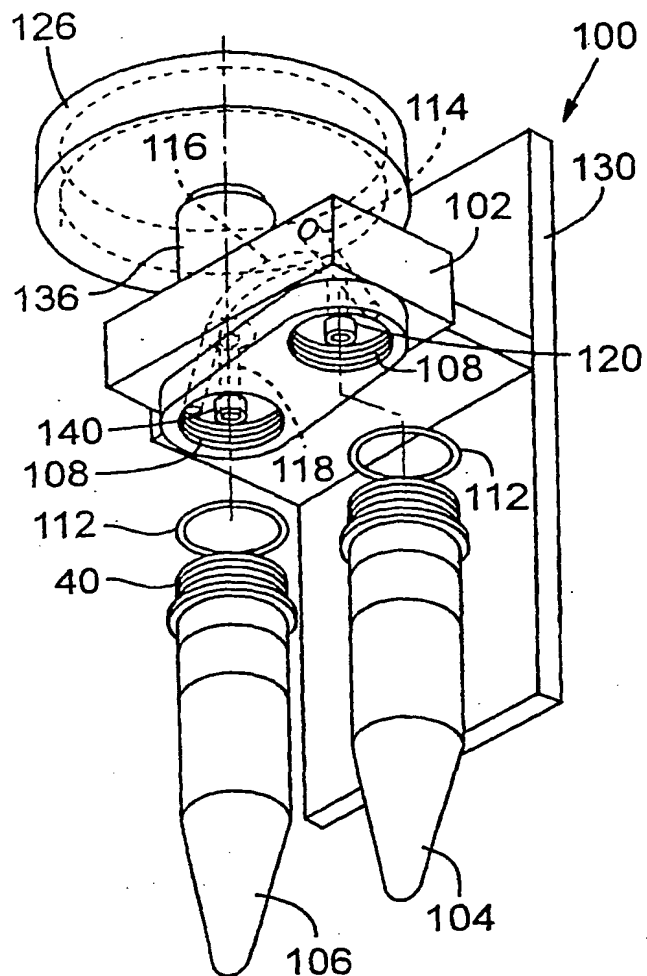


FIG. 9



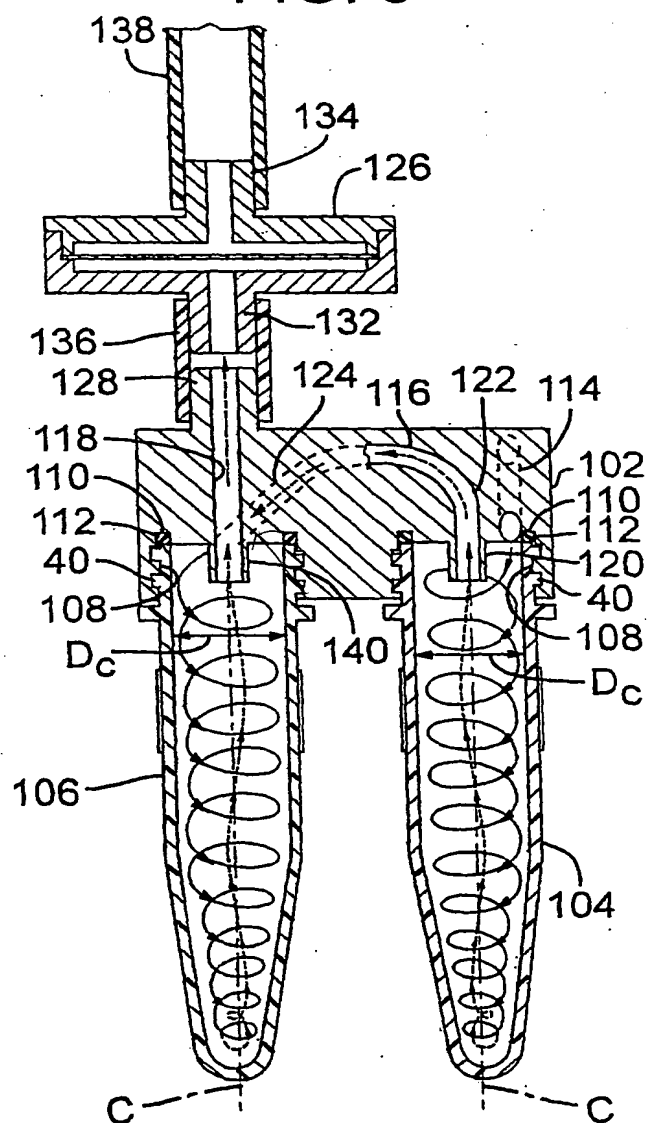


FIG. 10

Aspiration Efficiency of the Microtube Sampler
(error bar represents ± 1 SD; N=6)

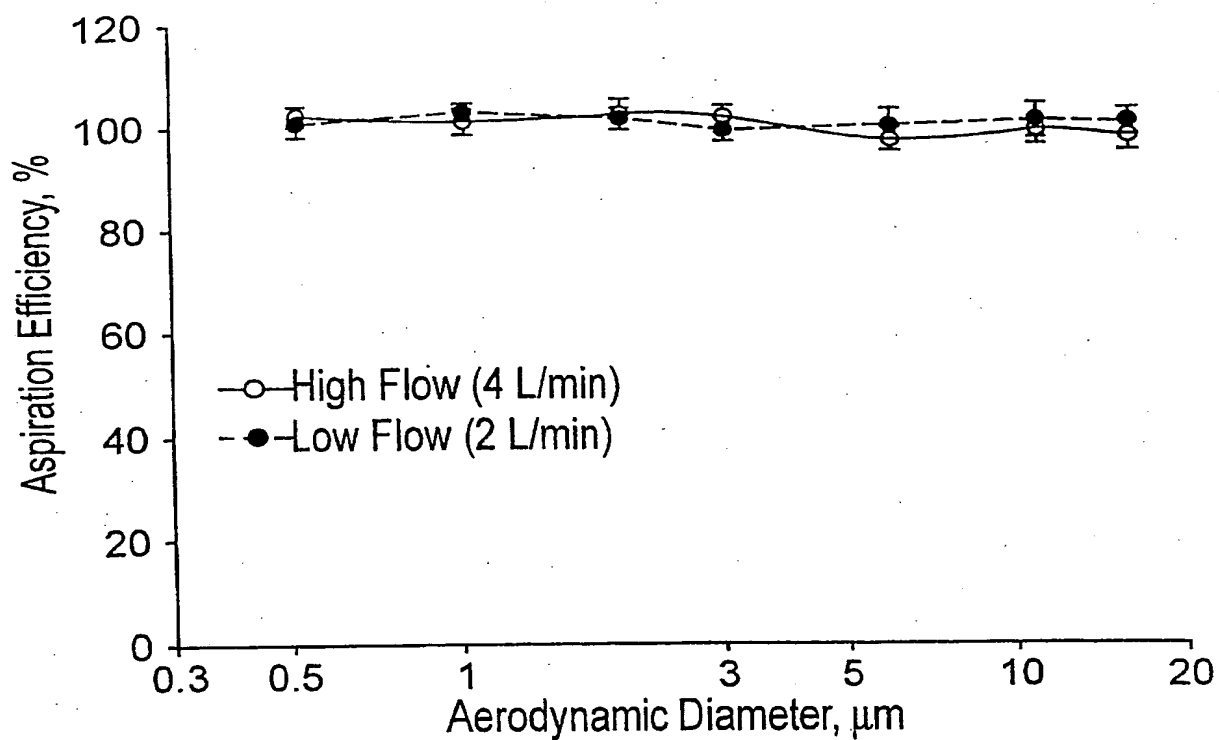

6/10

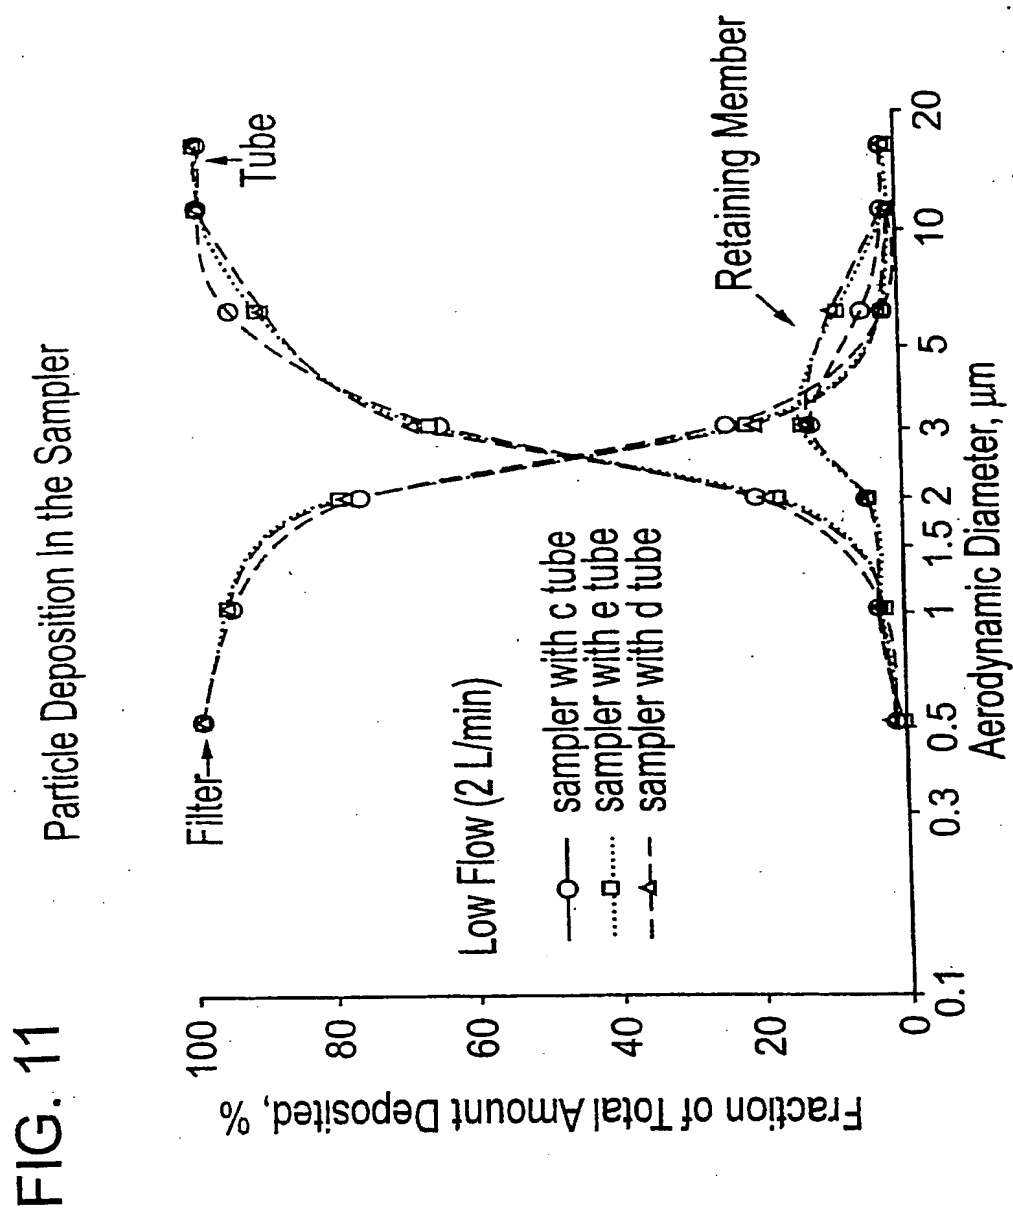

7/10

FIG. 12

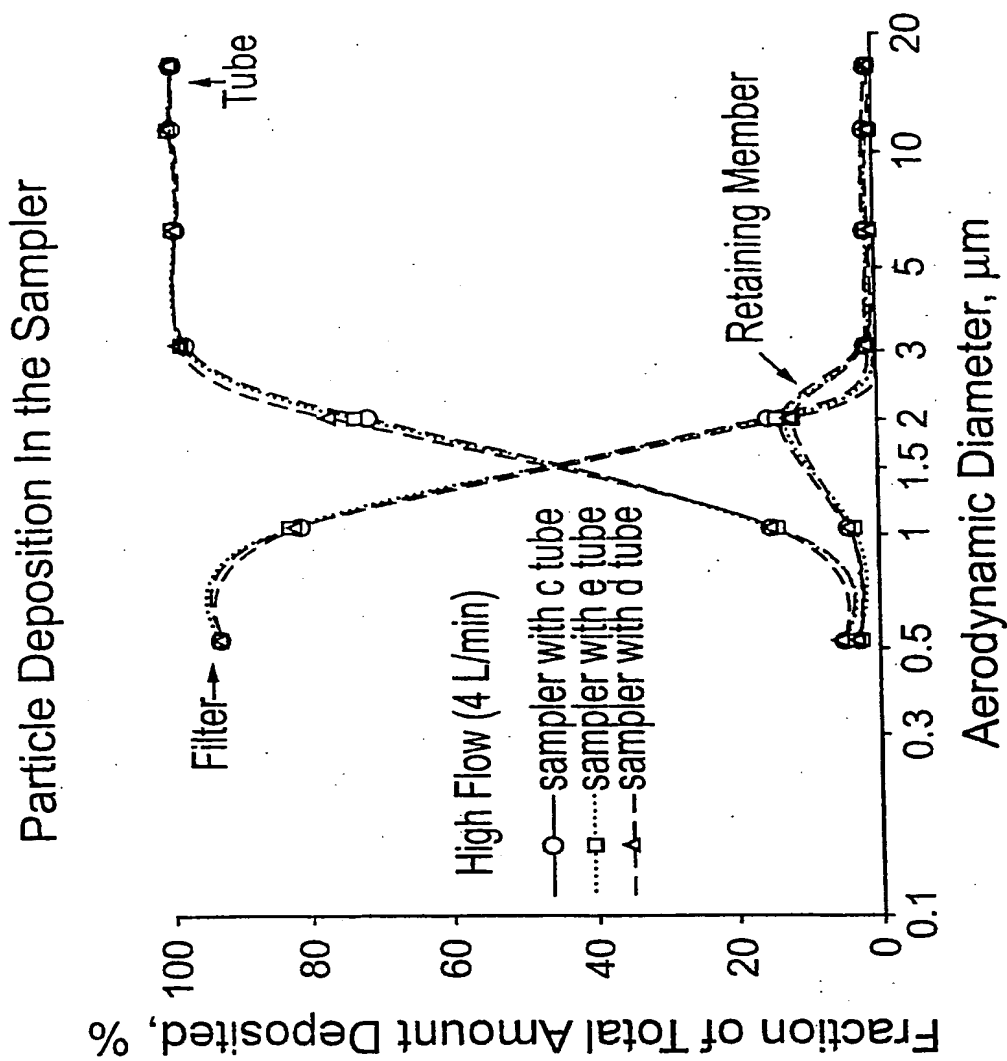


FIG. 13

Collection Efficiency of the Microtube Sampler ($D_{in} = 2\text{mm}$)
(Error Bar Represents $\pm 1\text{ SD}$; $N = 6$)


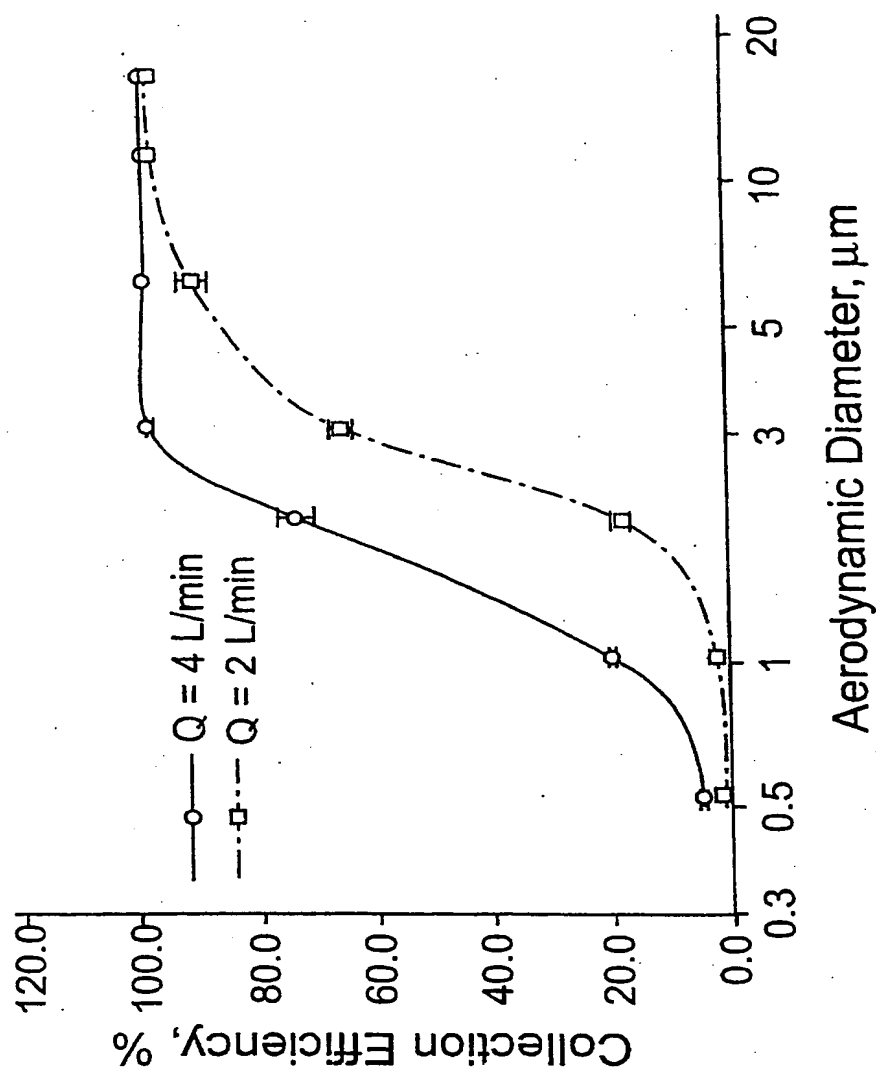


FIG. 14

Particle Collection Efficiency in the Tube



10/10

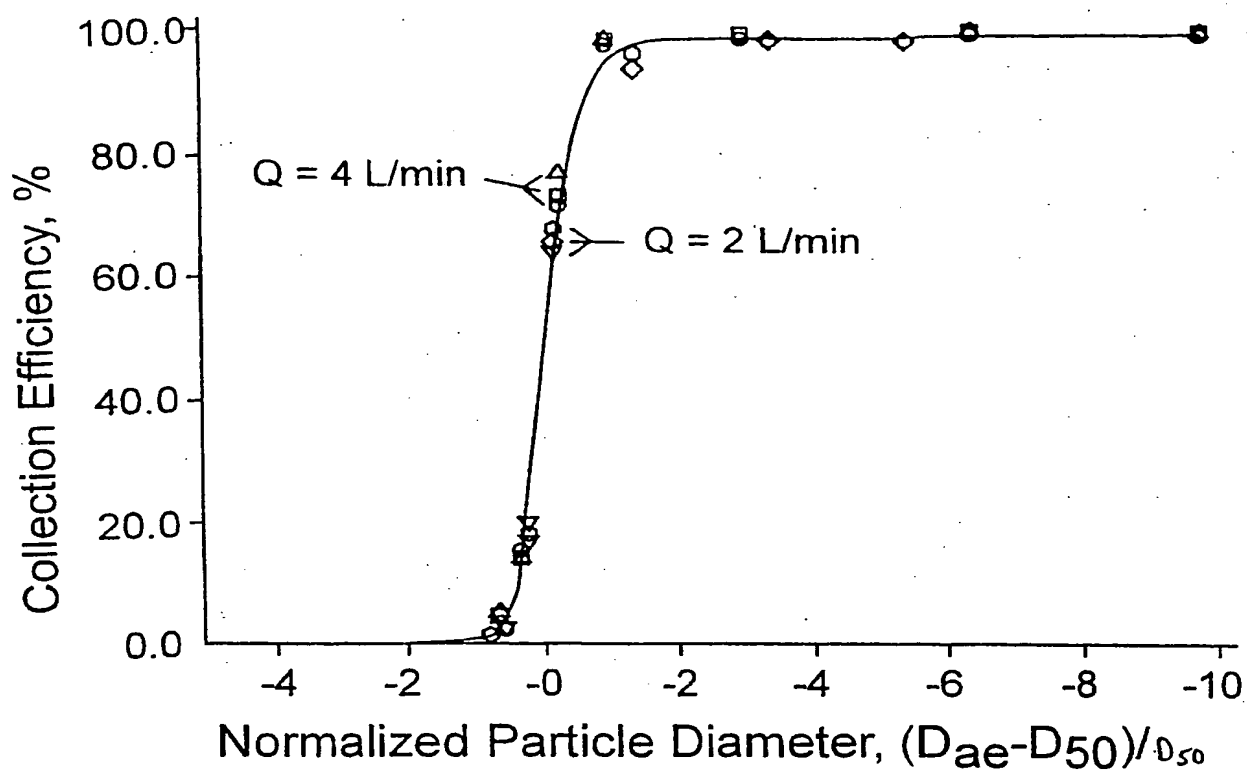